## **DEBRIS/ROUND CELL ASSESSMENT of SEMEN SAMPLES on the SQA**

## **OVERVIEW:**


Grading the degree of debris/round cells in semen samples run on the SQA Vision and SQA-iO is important because these components (that are the size of sperm heads or larger) can influence the accuracy of reporting automated concentration. This technical bulletin provides guidance for assessing/grading the % of sample debris/round cells by category.

## **ASSESSMENT TECHNIQUE:**

- 1. Debris/round cells are graded as a percentage in proportion to the number of sperm cells
- 2. Only particles without tails that are the size of sperm heads or larger should be counted as debris/round cells
- 3. Several fields may be required to estimate the % range of debris/round cells in the sample
- 4. The absolute number of debris/round cells is only important for determining the **percentage range of these components vs. sperm** and to properly select how to classify them by **category** (refer to table below)

#	% Range of Debris/Round Cells vs Sperm	Example	Debris Category in SQA
1	Less than 10%	# Sperm 50 and # Debris 1 = 2%	None/Few< 10%
2	10 to 30%	# Sperm 50 and # Debris 10 = 20%	<b>Moderate 10%-30%</b>
3	31 to 99%	# Sperm 50 and # Debris 30 = 60%	Many 31%-99%
4	≥ 100%	# Sperm 50 and # Debris 60 = 120%	Gross >=100%

# SAMPLE IMAGES with CATEGORIES of DEBRIS/ROUND CELLS

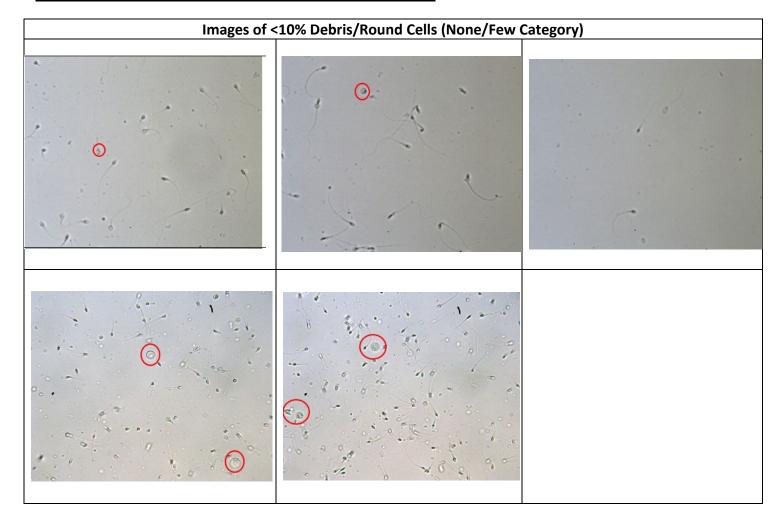



# Images of 10-30% Debris/Round Cells (Moderate Category) Images of 31-99% Debris/Round Cells (Many) Images of >= 100% Debris/Round Cells (Gross)

Distribution: All SQA Vision and SQA-iO distributors and users
Authority: Dr. Lev Rabinovitch, CTO Emeritus / Marcia Deutsch CEO
www.mes-global.com