

Technical Release Bulletin: QwikCheck™ Test Strips

(For SQA-V software version 2.43 through 2.49 Gold)


Issue date: Wednesday, November 04, 2009

Subject: QwikCheck™ Test Strips – pH labeling on Lot # 20074_200709 and 19776_200709


Background: QwikCheck™ Test Strips are used to assay pH and WBC levels in semen. The outside label provides ranges for pH based on a color chart.

Update: The pH color chart for LOT #20074_200709 and 09776_200709 are missing the numerical ranges.

Procedure for LOT # 20074_200709: Please use the color chart and numerical ranges below as a guideline for pH:

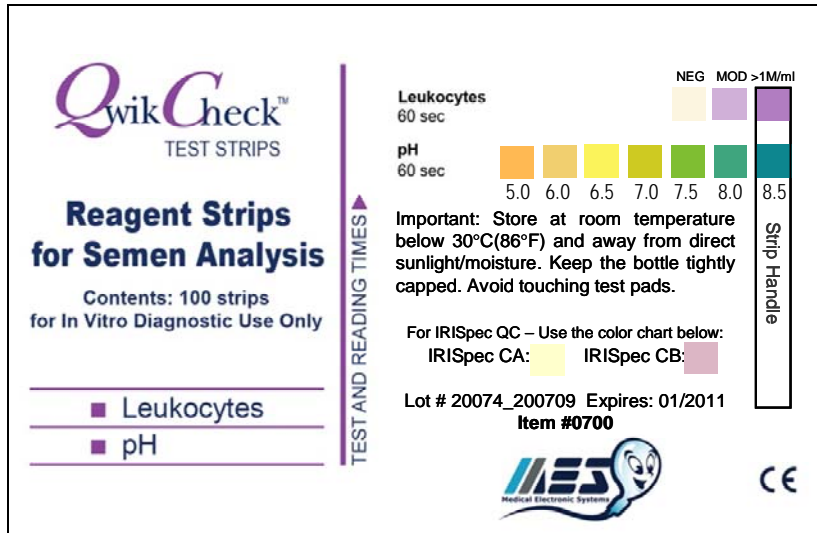

Procedure for LOT # 19776_200709: Please use the color chart and numerical ranges below as a guideline for pH:

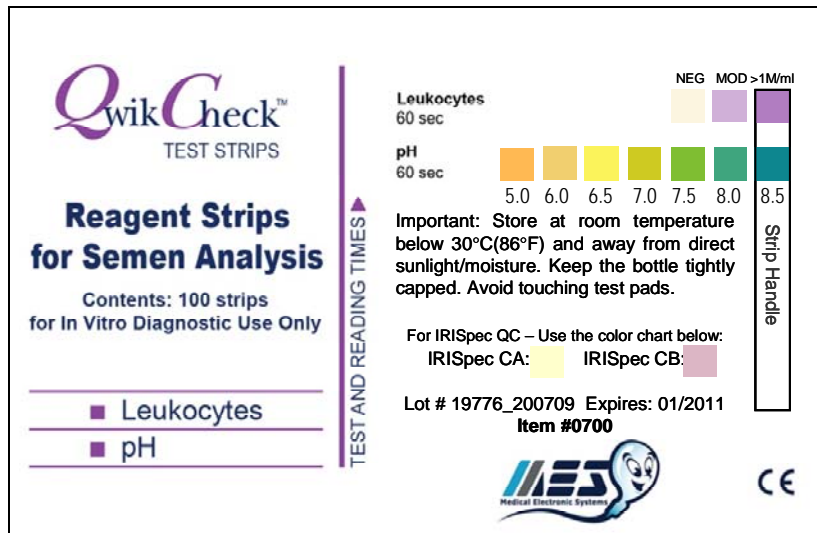

Distribution:
Effective Date:
Approval:

U.S. and on demand
Immediate, Wednesday, November 04, 2009
Dr. Lev Rabinovitch, CTO



www.mes-ltd.com Tel: 972-4-637-3981 Fax: 972-4-637-3984

Technical Release QwikCheck™ Test Strips